
# Liberty united with stay-safe

# How to Insert the Liberty® Cycler Cassette

**Note:** This document is not intended to replace your doctor's or peritoneal dialysis nurse's advice or training. Please refer to your Liberty cycler's user guide for more information on how to safely and effectively use your Liberty cycler.

#### **Step 1: Prepare the Cassette**

When prompted on the cycler screen to "insert cassette" ...




- Remove the cycler set from its packaging.
- Inspect the cycler set to make sure it's free from kinks or damage. Look for scratches, loose tubing, or small holes in the cassette film.



**Caution:** Use caution when touching the cassette film to prevent damage.




**Warning:** DO NOT USE the set if it is damaged. Put the damaged set aside and immediately call Customer Service at 800-323-5188 to arrange a pick-up to return the damaged set.



Sample cycler set with cassette and tubing


### Step 2: Open the Cassette Door

Firmly push the door latch to open the cassette door.





**Caution:** The cassette door is pressurized. Do not attempt to open the cassette door until your machine instructs you to do so.

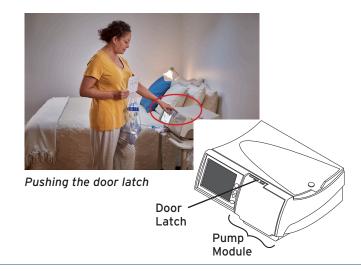

### **Step 3: Insert the Cassette**

Hold the cassette with the plastic domes facing outward (towards you).

Slide the cassette up and under the metal guide

pins at the top of both sides of the pump module.




Cassette Domes

Guide Pins

Guide Pins

Inserting the cassette

Then, snap the cassette in place using the catch at the bottom of the pump module.

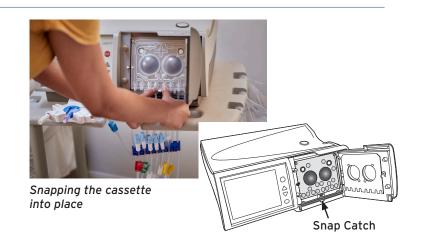

#### If your cycler has an alignment bar...

- Make sure the cassette is resting up and under both guide pins.
- Make sure the bottom of the cassette is snapped in place and resting on the catch.
- The tubing should hang down in front of the cycler over the alignment bar.



Cycler with alignment bar

#### If your cycler DOESN'T have an alignment bar...

- Make sure the cassette is resting under the guide pins at the top of the pump module and within the snap catch at the bottom of the pump module.
- The tubing should hang freely down in front of the cycler.



Cycler without alignment bar

## Step 4: Close the Cassette Door

Close the door over the cassette. Ensure the cassette door clicks into place to lock it.




**Caution:** Do NOT force the door closed. If you're having trouble closing the door, open the cassette door and make sure the cassette has been inserted correctly (see Step 3).

Your cycler will pressurize the cassette door and then display the next step of the setup process.



**Warning:** A damaged cassette can cause peritoneal dialysis (PD) solution to leak into the cycler and is a potential risk for contamination. Notify your PD nurse if you find a fluid leak.



**Indications for Use:** The Liberty, Liberty Select, and Liberty PDx cyclers are indicated for acute and chronic peritoneal dialysis.

**Caution:** Federal (US) law restricts these devices to sale by or on the order of a physician.

**Note:** Read the Instructions for Use for safe and proper use of these devices. For a complete description of hazards, contraindications, side effects, and precautions, see full package labeling at www.fmcna.com.







© 2019 Fresenius Medical Care. All Rights Reserved. Fresenius Medical Care, the triangle logo, Liberty, Liberty Select, and Liberty PDx are trademarks of Fresenius Medical Care Holdings, Inc. or its affiliated companies. All other trademarks are the property of their respective owners. P/N 71-4593.B